



ELUTION VOLUME (x5ml, Tris-HCl BUFFER, pH7.0)


FIG. 1

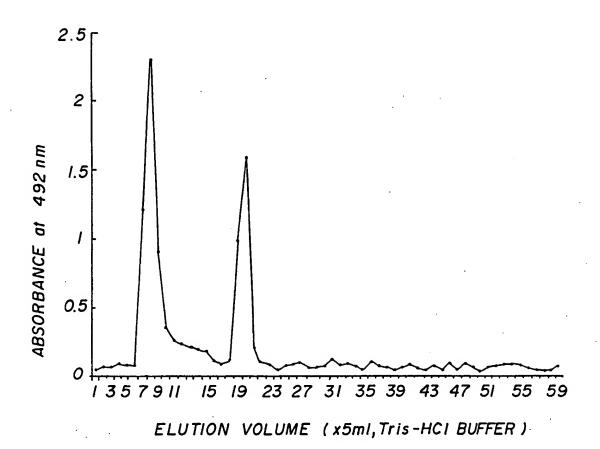


F1G. 2

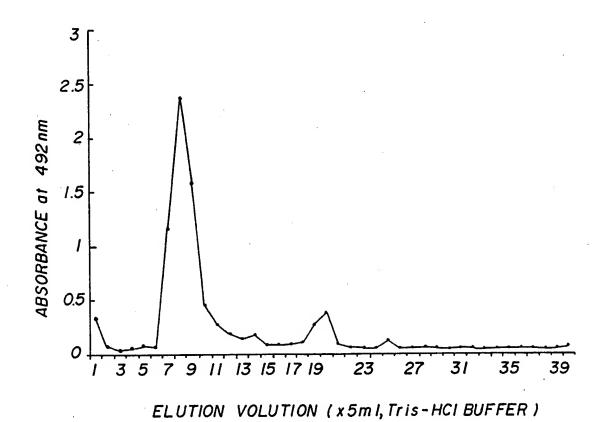


F1G. 3

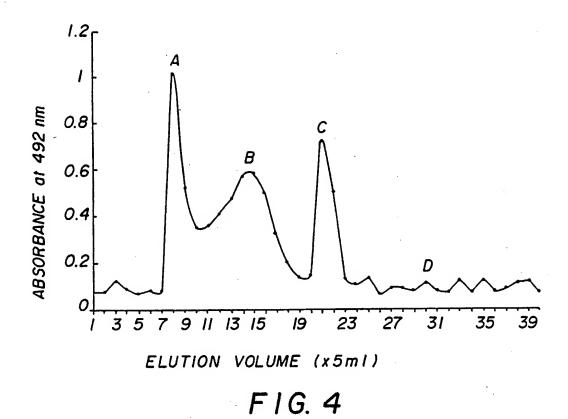

SUBSTITUTE SHEET (RULE 26)

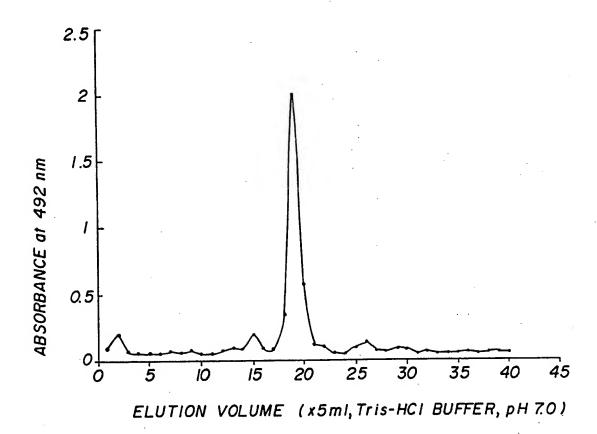


F1G. 5

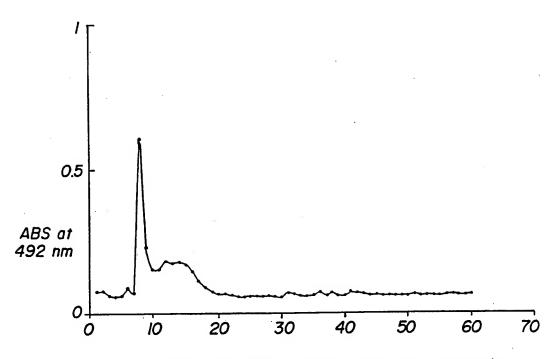


ELUTION VOLUME (x5ml, Tris-HCl BUFFER)

F1G. 6

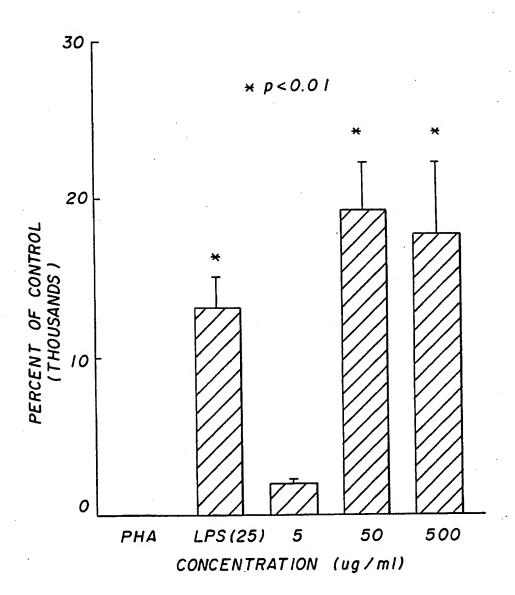

F1G. 7

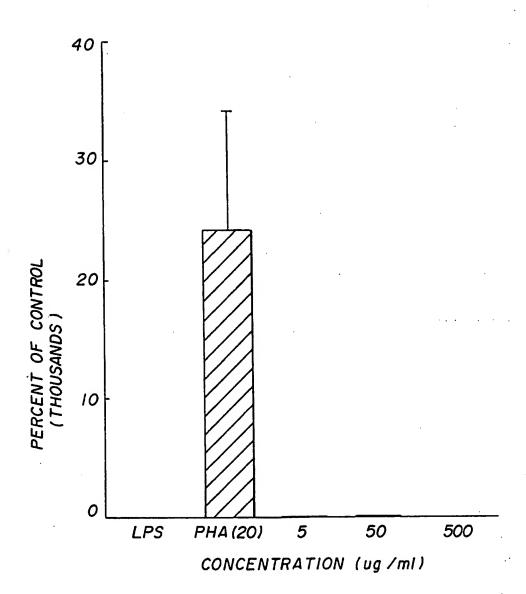

F1G. 8

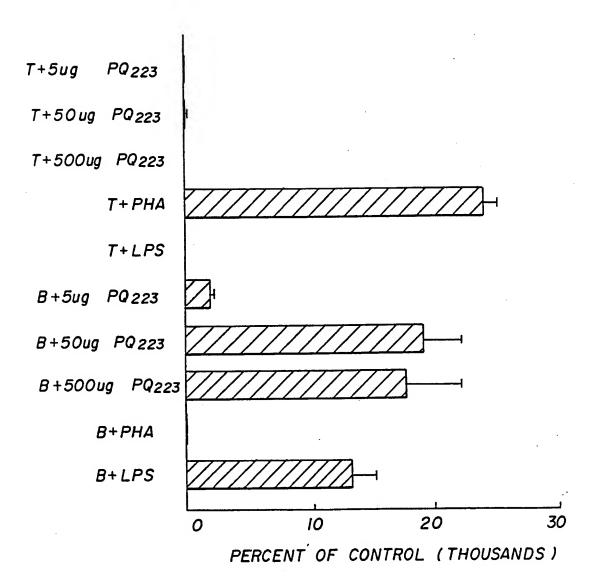


FIG. 9

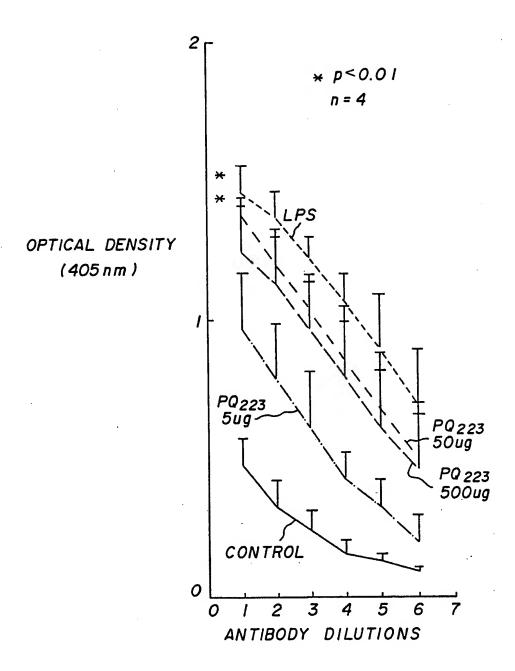


FIG. 10

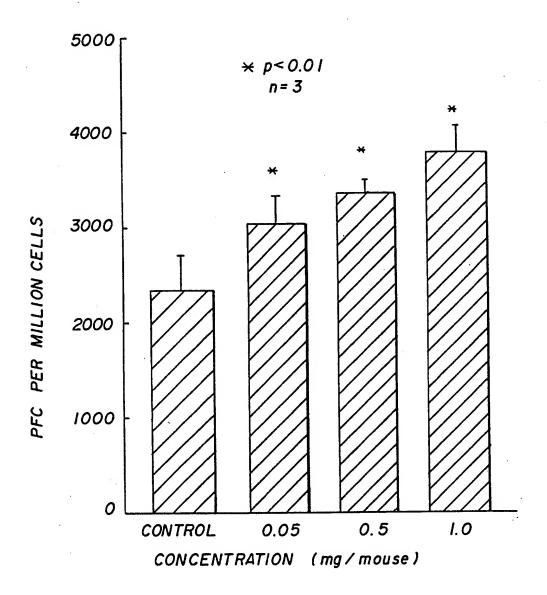


FIG. 11